

0528294-05201

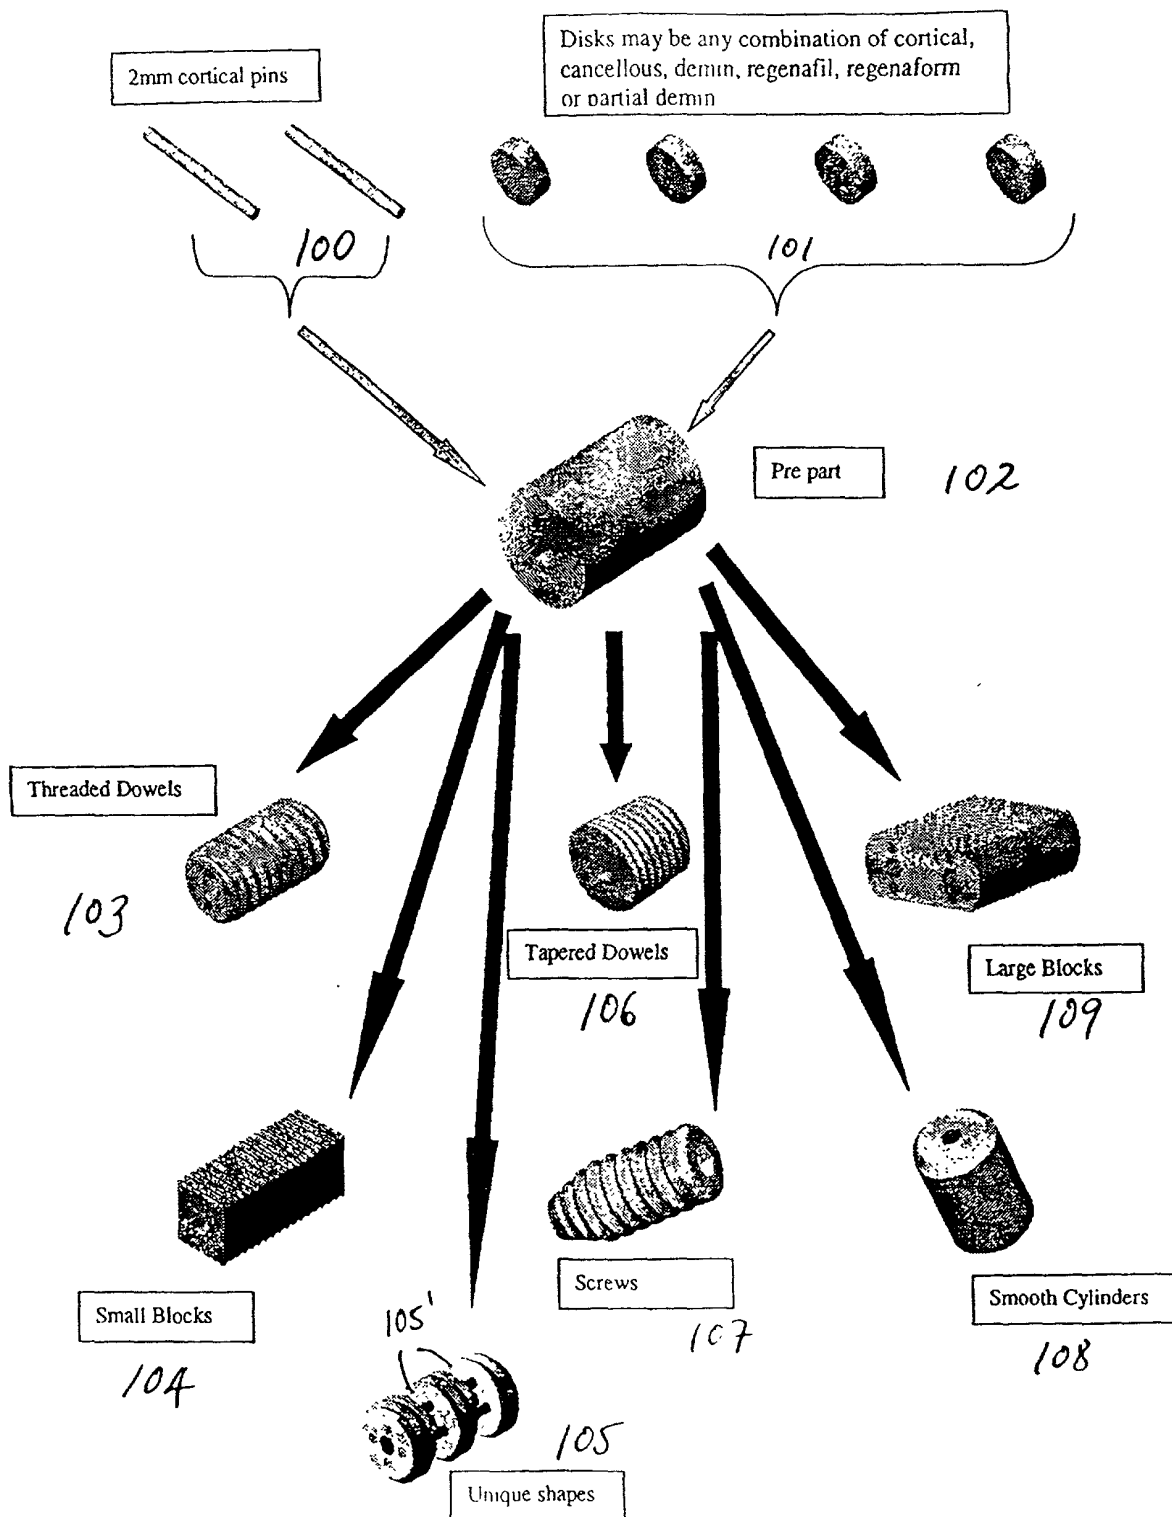


Figure 1

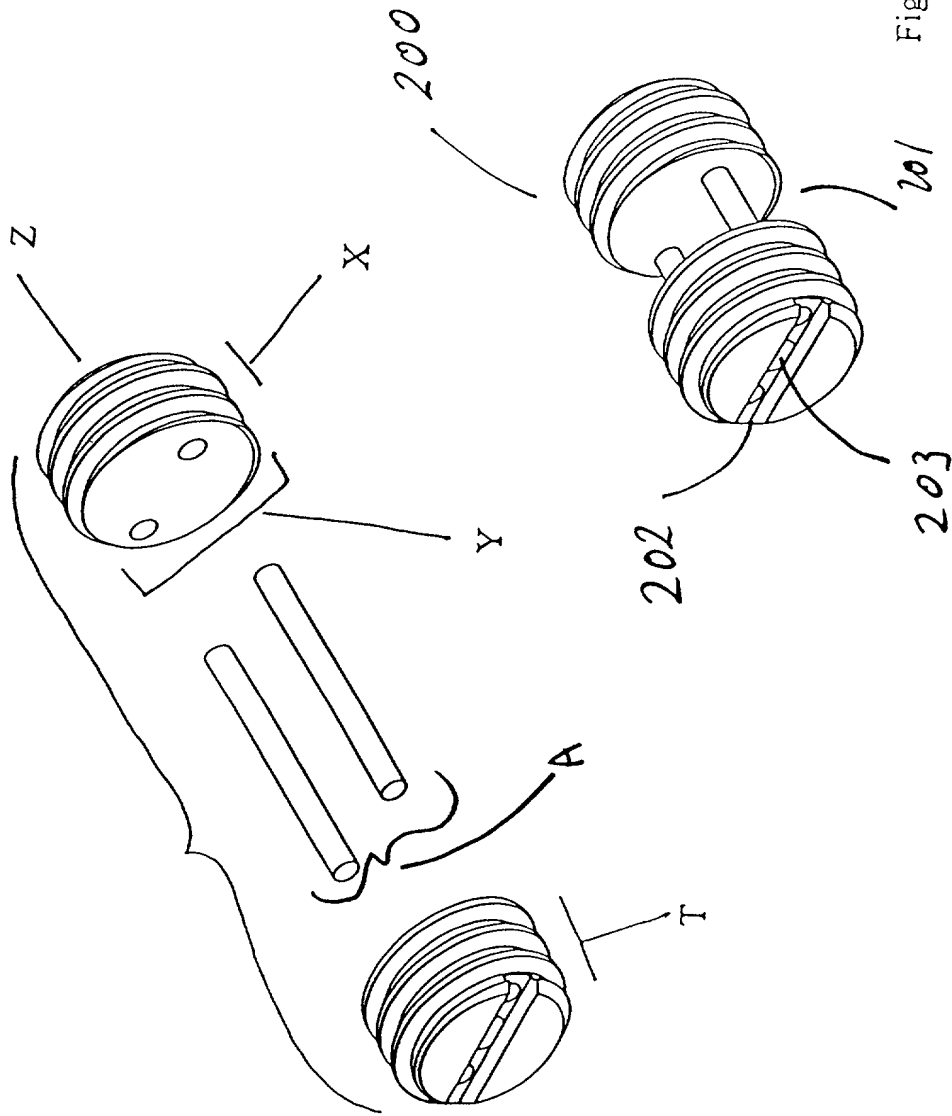


Figure 2

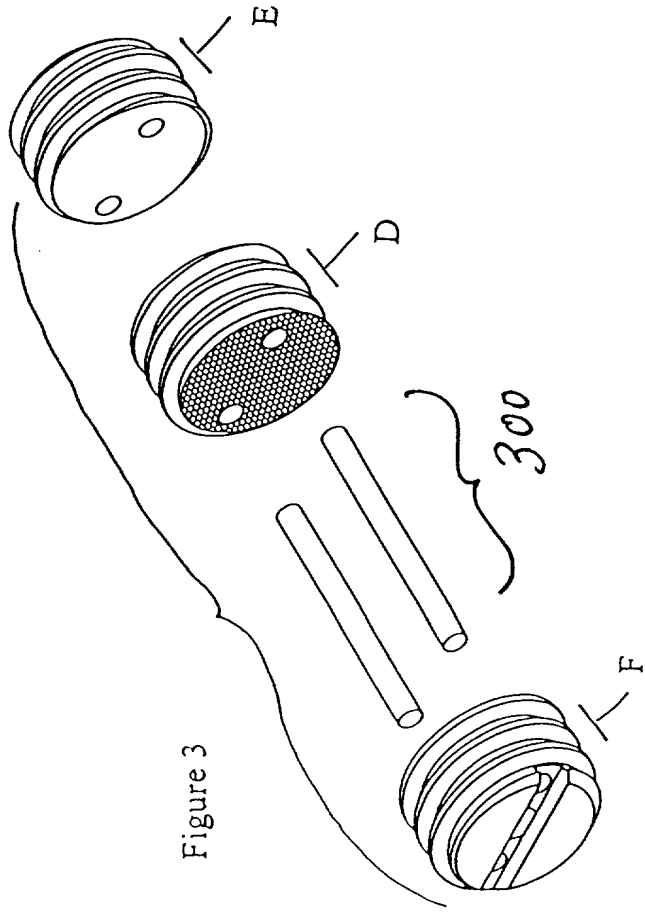


Figure 3

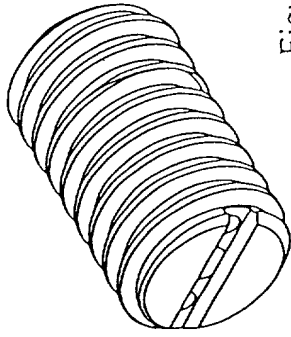


Figure 4

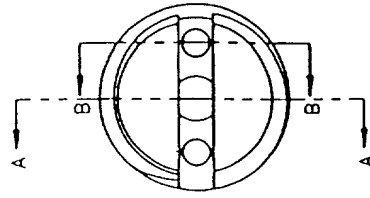


Figure 5

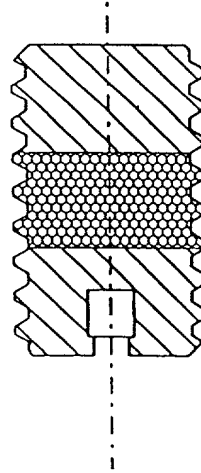


Figure 6

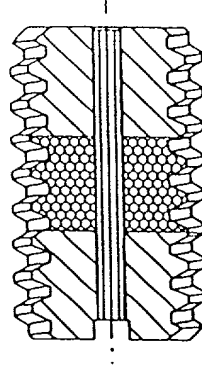
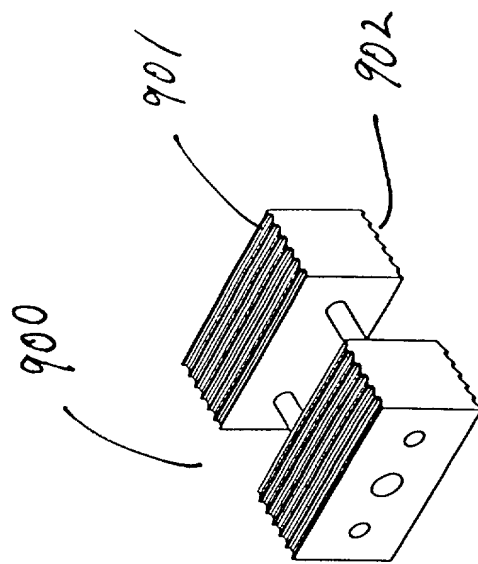
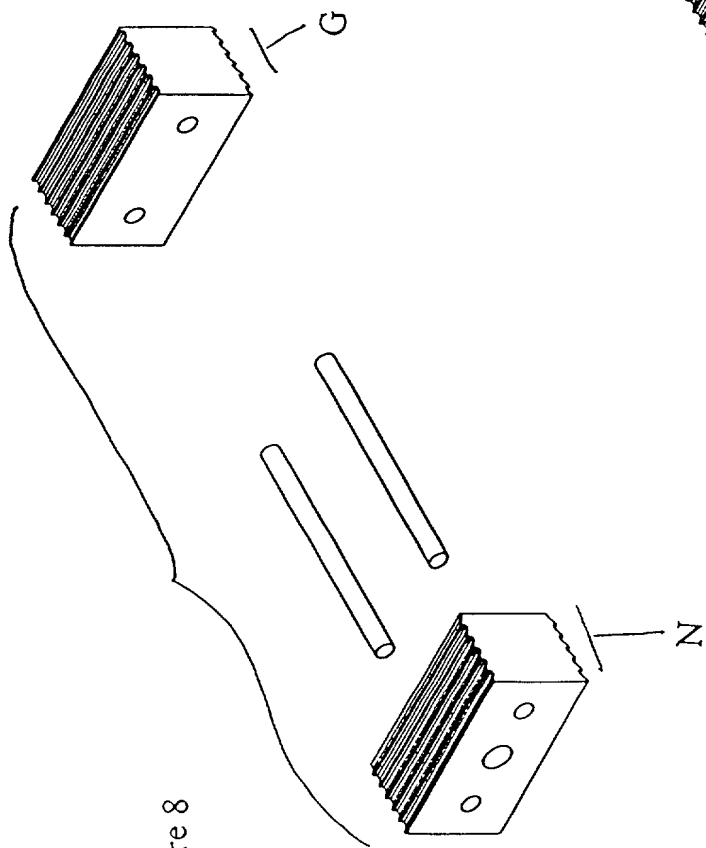


Figure 7



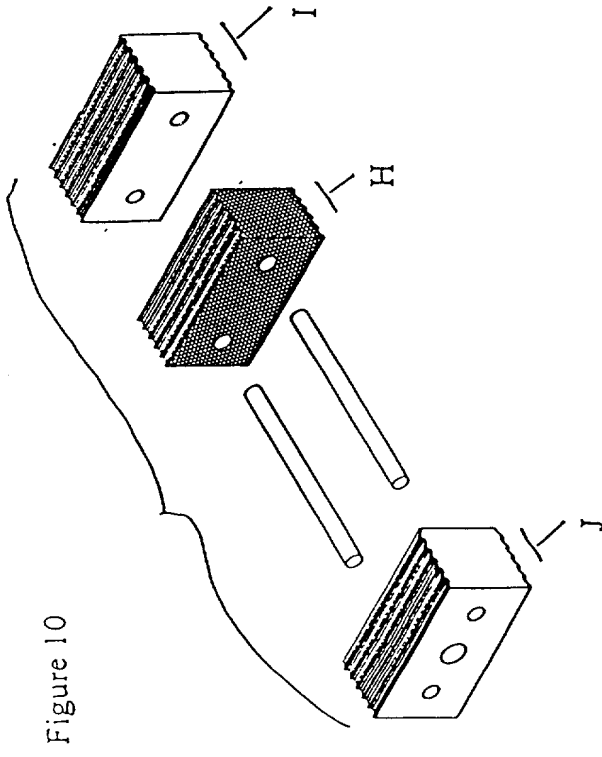


Figure 10

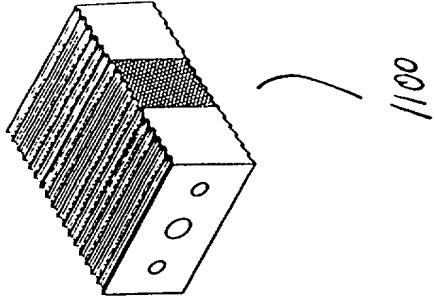


Figure 11

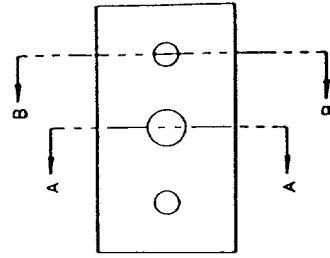
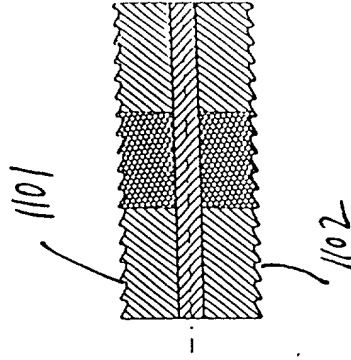


Figure 12

Figure 13

Figure 14

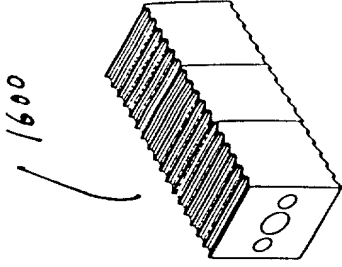
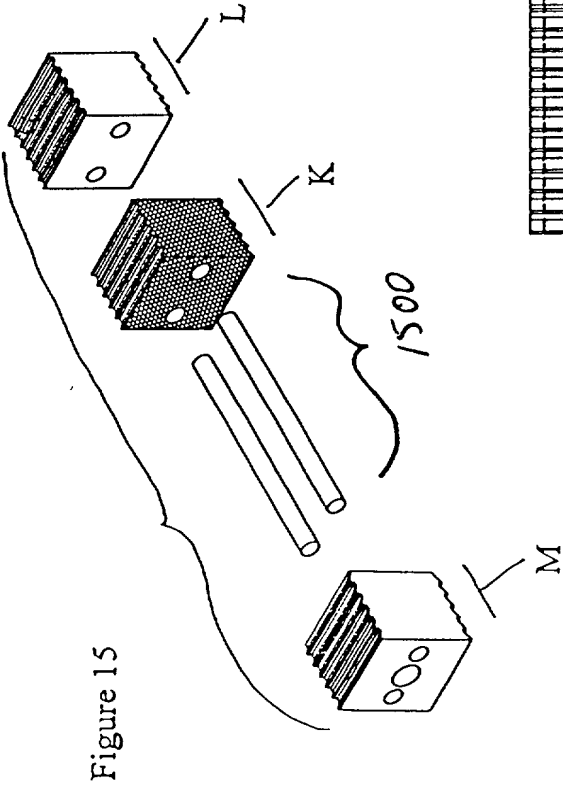


Figure 16

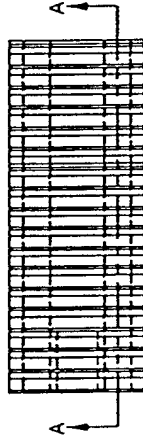


Figure 17

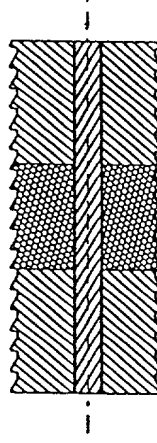


Figure 18

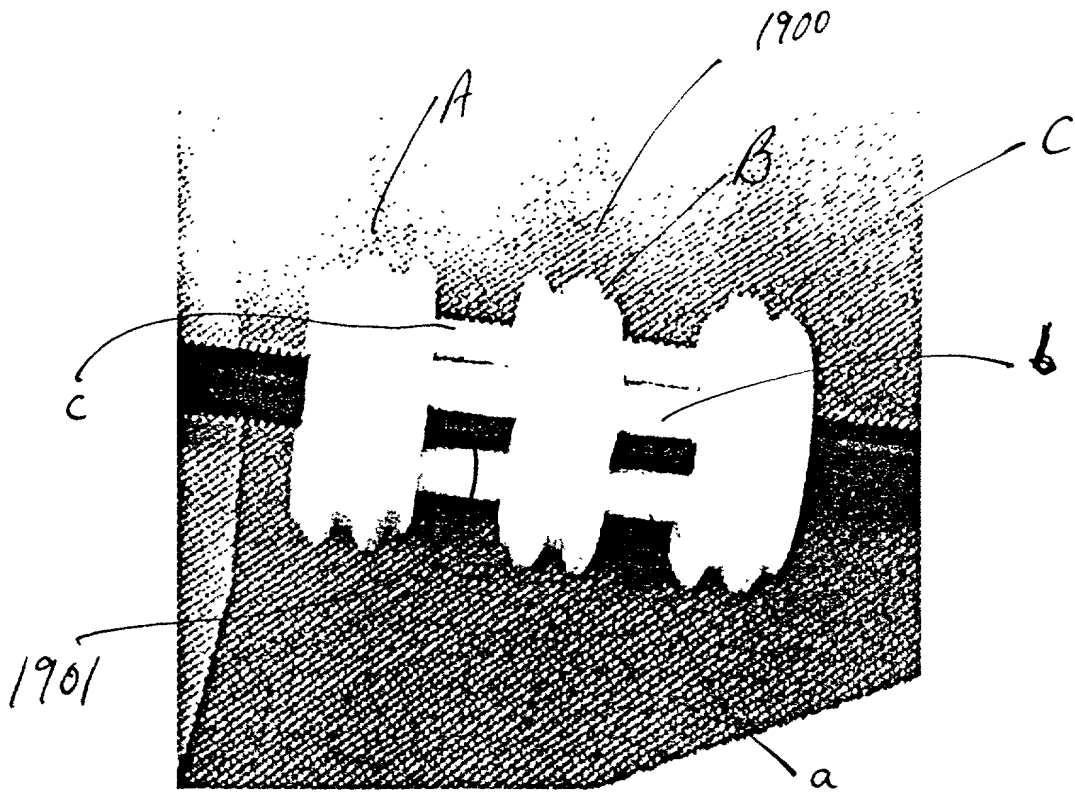


FIGURE 19

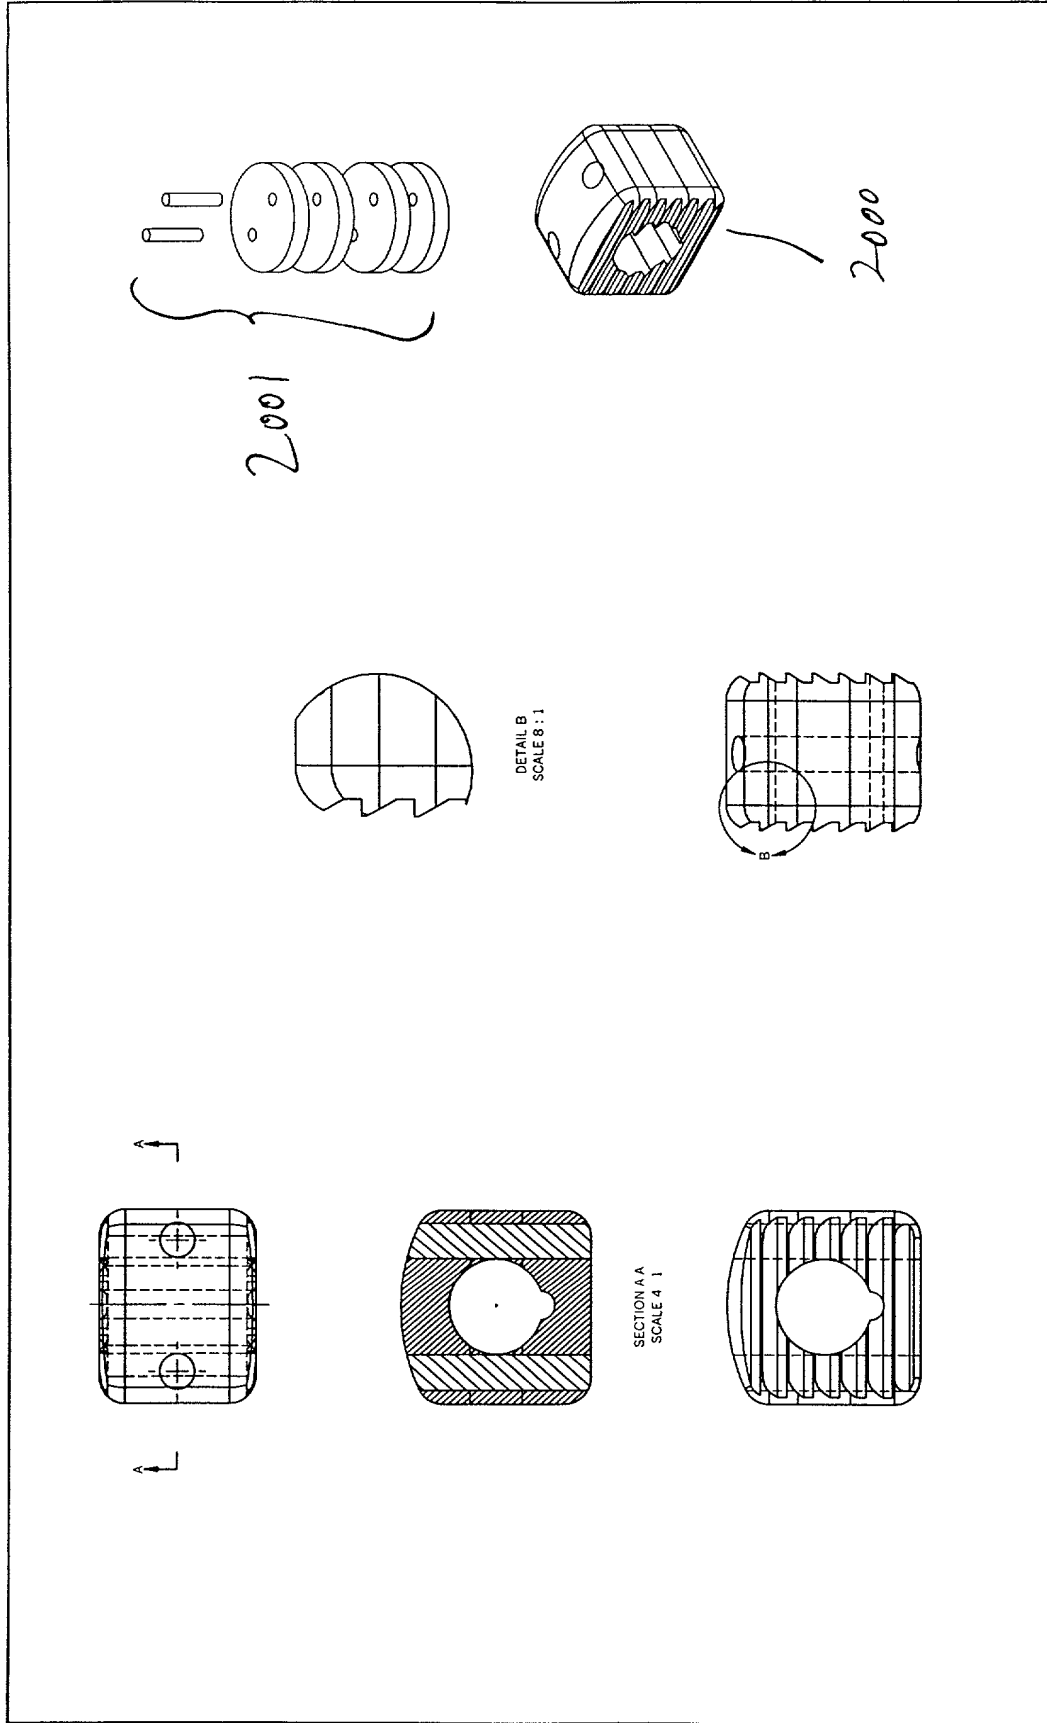


Figure 20



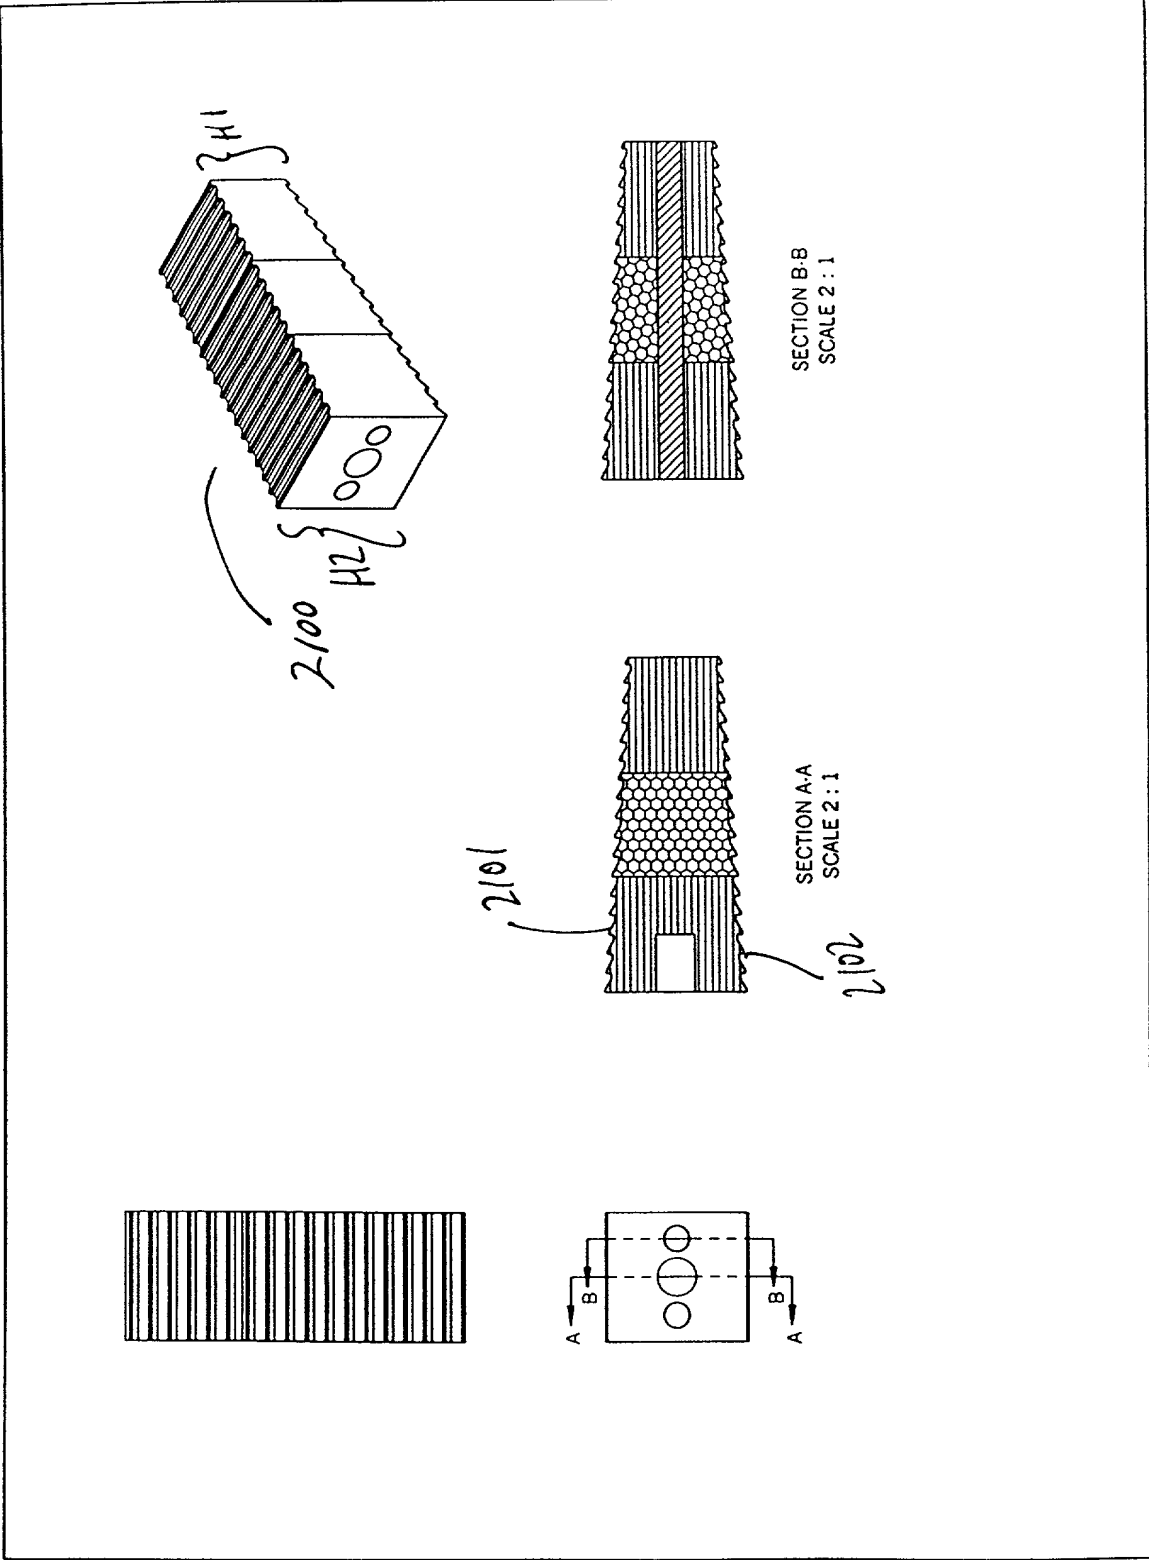


Figure 21


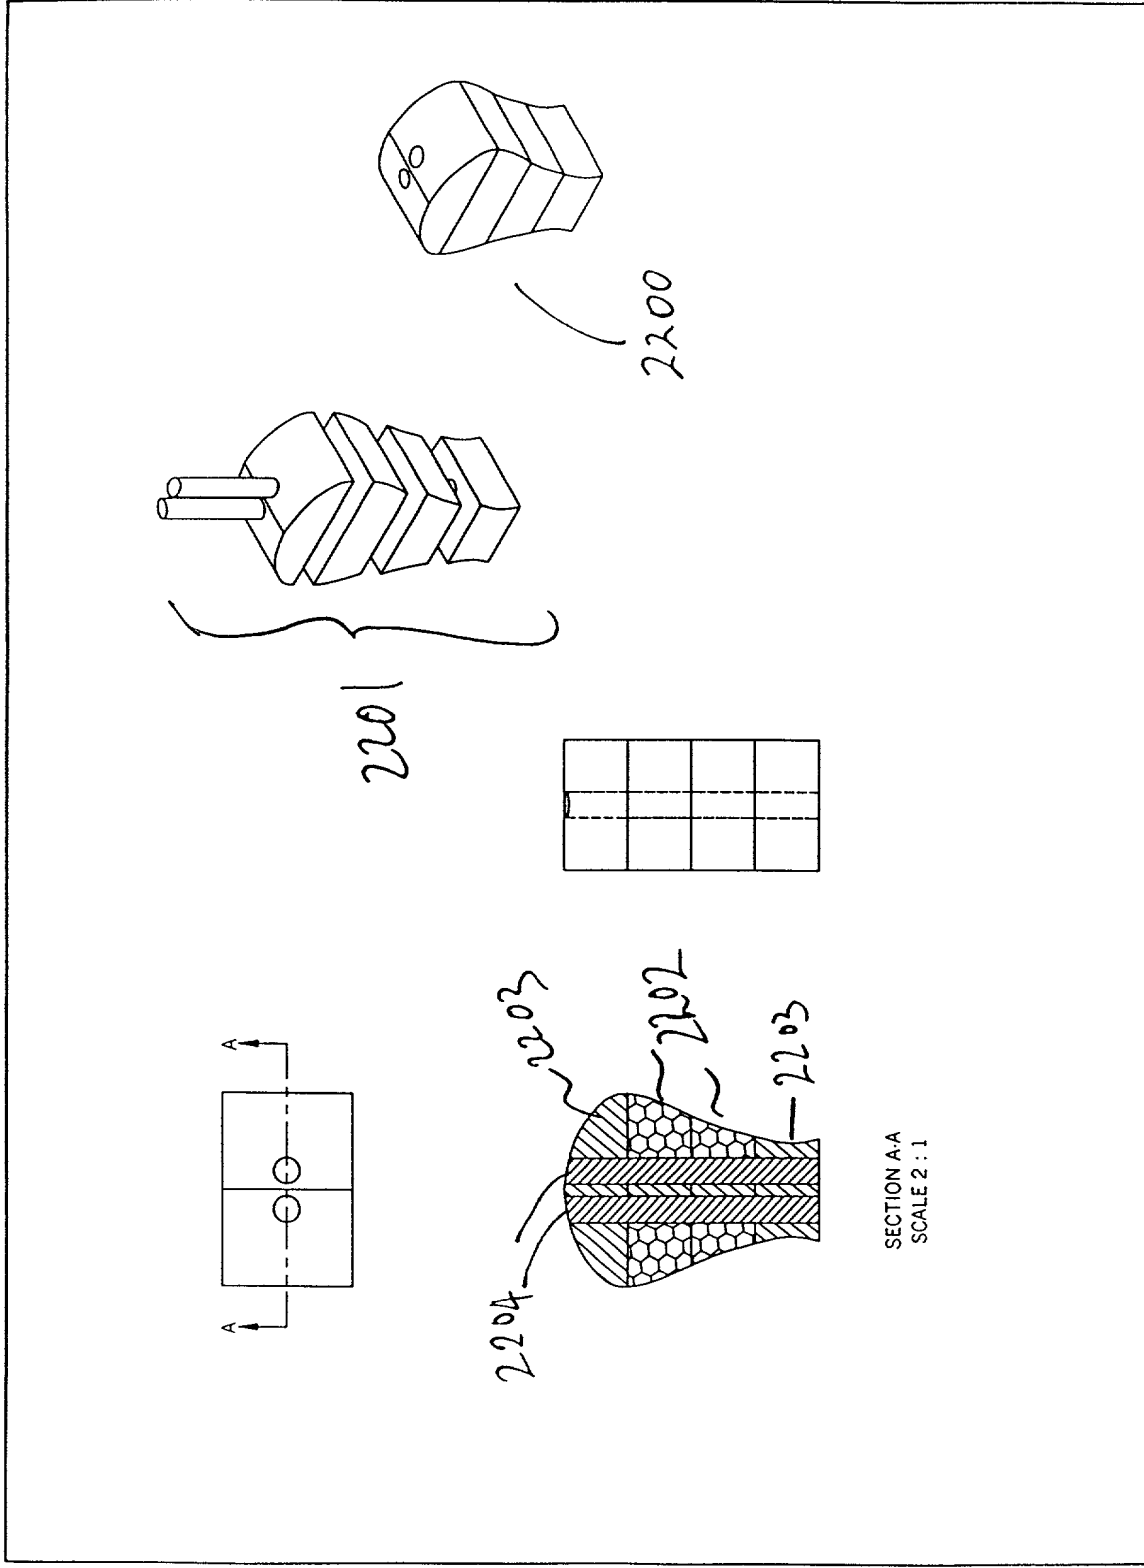



Figure 22

Figure 23

Create a tapered dowel

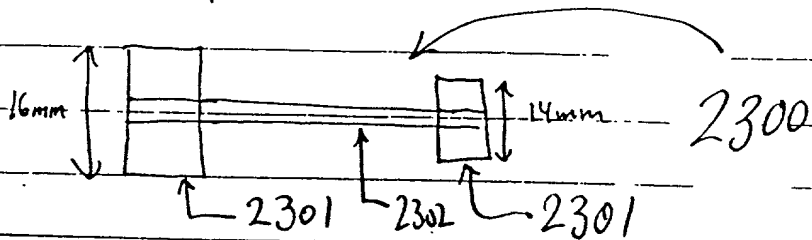

Salvage dowel out of spec

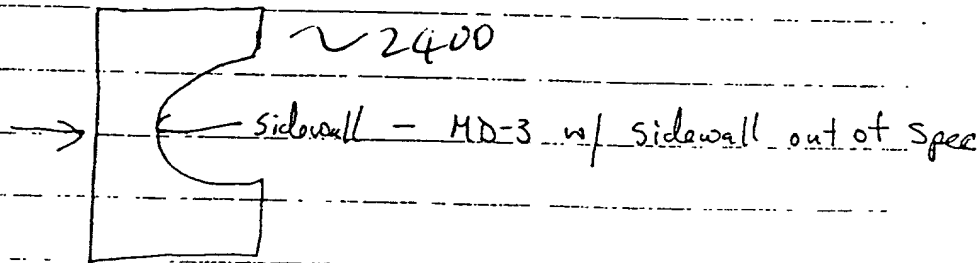

Solution - Create an MD-2 Figure 24A


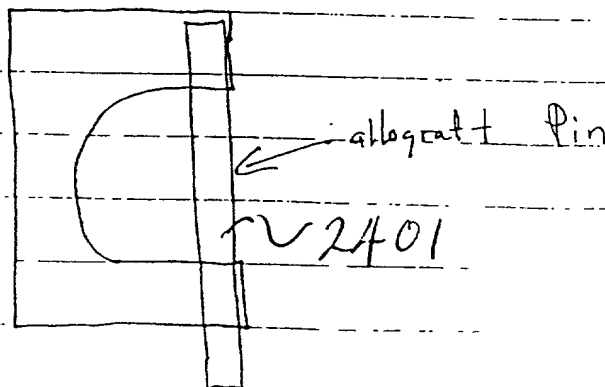


Figure 24B

Figure 24

09783594-059501

Figure 25

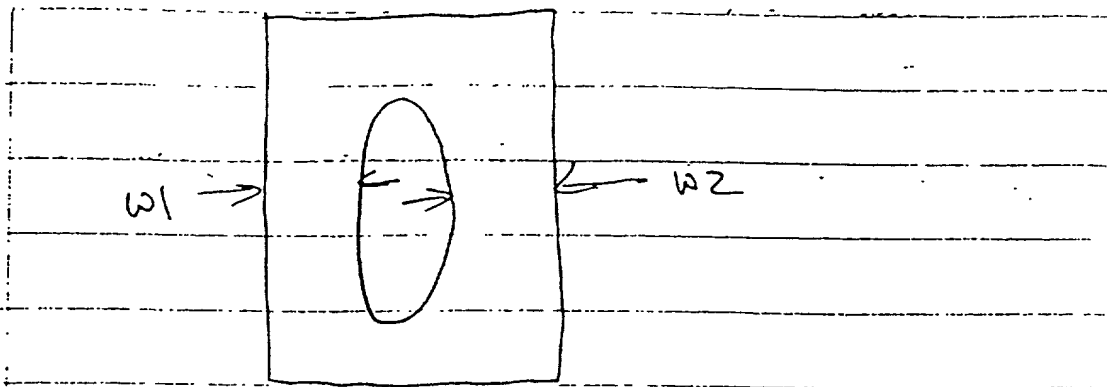

MD-2 out of spec @ sidewall


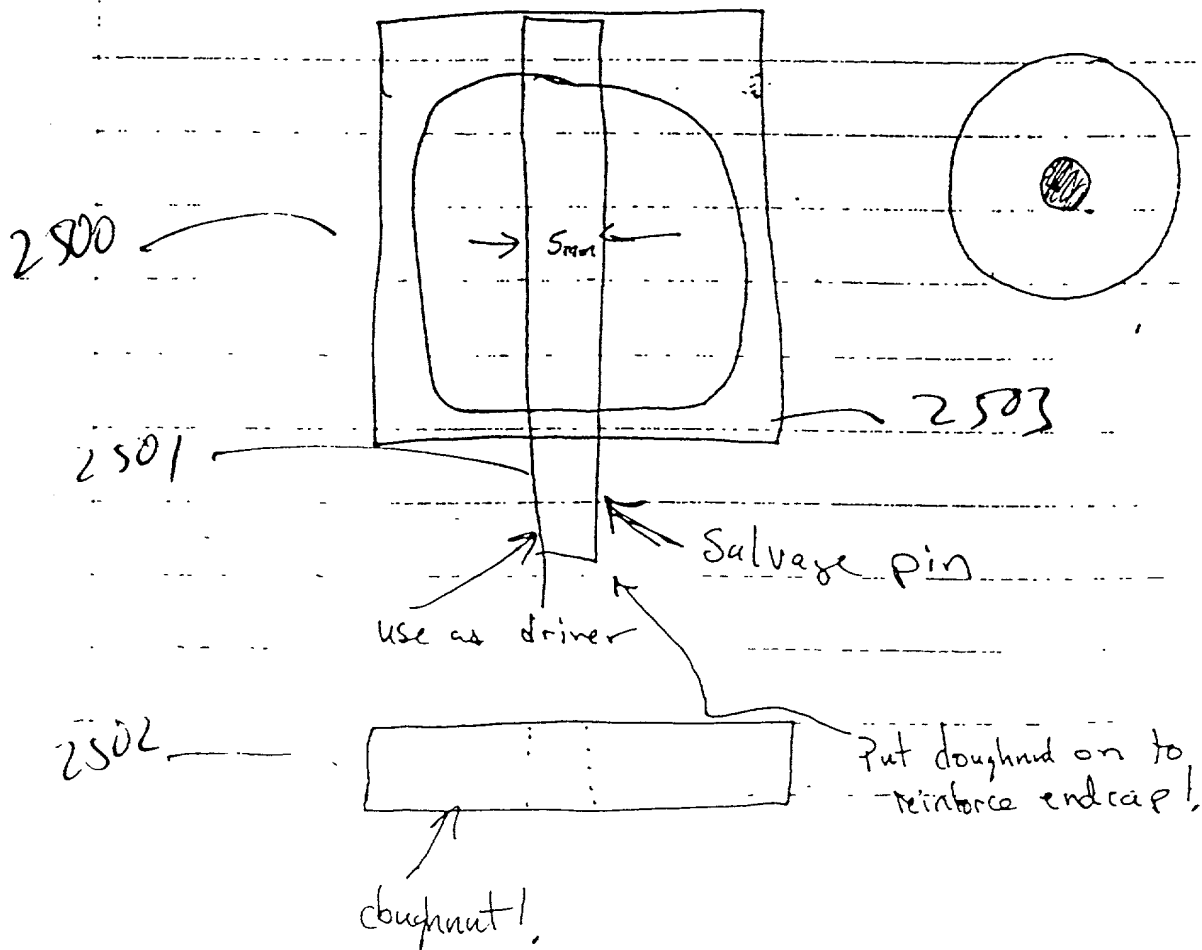


Figure 26


Cancellous bone

2600




12 x 2mm


Cortical Pins 100




6 x 2mm




9 x 3mm



12 x 3mm



6 x 3mm



6 x 4mm

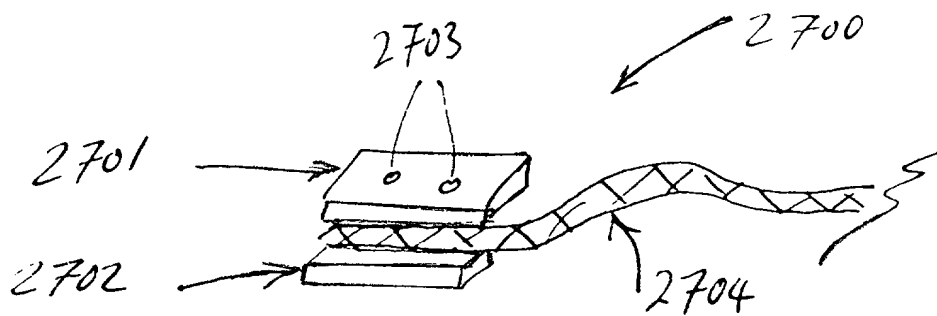


Figure 27